

Replace Outlet valve


Instructions

Scope

Instructions how to replace Outlet valve V9-O (28956512) or Outlet valve V9H-O (28979281).

Location and illustration of Outlet valve

The illustration below shows the location of the Outlet valve and also an enlargement of the valve. In ÄKTA™ avant 25, the Outlet valve is labelled **V9-O**. In ÄKTA avant 150, the Outlet valve is labelled **V9H-O**.

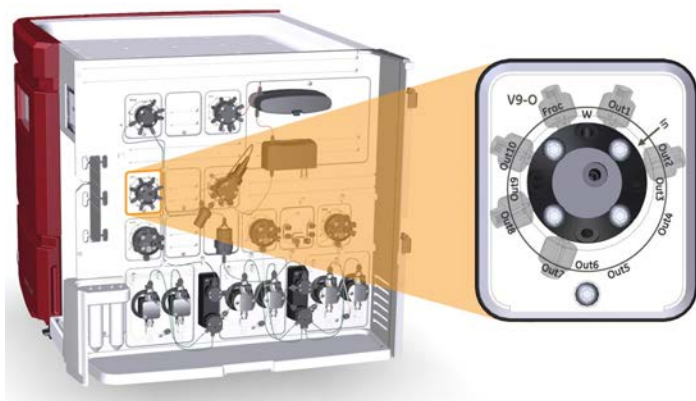

Instruction

The instruction below describes how to replace a valve module in the instrument.

Note: *The illustrations show the principle how to replace a valve. The position of the valve on the instrument and the used type of valve will depend on the valve being replaced.*



WARNING

Disconnect power. Always switch off power to the instrument before replacing any component on the instrument, unless stated otherwise in the user documentation.

Step	Action
1	Disconnect power from the instrument by switching off the instrument with the Power switch located on the left hand side of the instrument.
2	Loosen the valve module with a Torx screwdriver.




- 3 Remove the valve module.



Step	Action
------	--------

- | | |
|---|---|
| 4 | Disconnect the cable and secure it in the slit. |
|---|---|

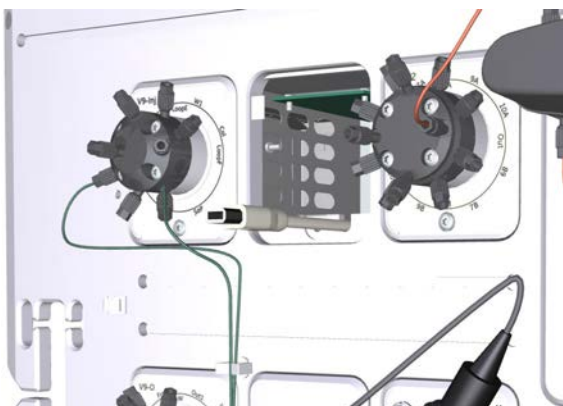

- | | |
|---|--|
| 5 | Connect the cable to the new valve module. |
|---|--|



- | | |
|---|--------------------------|
| 6 | Insert the valve module. |
|---|--------------------------|




Step	Action
7	Fasten it with a Torx screwdriver.



Connect tubing

The illustration below shows the ports of the Outlet valve.

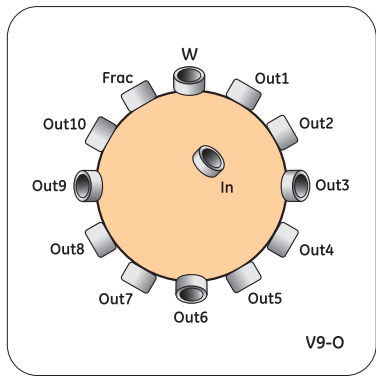

Port	Description		
In	Inlet port	Out1 - Out10	Outlet ports 1 - 10
Frac	Port to Fraction collector	W	Waste port

Page intentionally left blank



cytiva.com/AKTA

Cytiva and the Drop logo are trademarks of Global Life Sciences IP Holdco LLC or an affiliate.

AKTA is a trademark of Global Life Sciences Solutions USA LLC or an affiliate doing business as Cytiva.

All other third-party trademarks are the property of their respective owners.

© 2020–2021 Cytiva

All goods and services are sold subject to the terms and conditions of sale of the supplying company operating within the Cytiva business. A copy of those terms and conditions is available on request. Contact your local Cytiva representative for the most current information.

For local office contact information, visit cytiva.com/contact

28968646 AC V:4 01/2021